

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : C07K 14/00	A2	(11) International Publication Number: WO 00/11024 (43) International Publication Date: 2 March 2000 (02.03.00)
(21) International Application Number: PCT/US99/19374 (22) International Filing Date: 20 August 1999 (20.08.99) (30) Priority Data: 60/097,506 21 August 1998 (21.08.98) US (71) Applicant: SURROMED [US/US]; 1060 East Meadow Circle, Palo Alto, CA 94303 (US). (72) Inventors: DIETZ, Louis, J.; 550 S. Shoreline Boulevard, Mountain View, CA 94041 (US). WALTON, Ian; 346 Lakeview Way, Redwood City, CA 94062 (US). NORTON, Scott; 600 Rainbow Drive, #149, Mountain View, CA 94041 (US). (74) Agents: SWANSON, Barry, J. et al.; Swanson & Bratschun, L.L.C., Suite 200, 8400 E. Prentice Avenue, Englewood, CO 80111 (US).		(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>Without international search report and to be republished upon receipt of that report.</i>
(54) Title: NOVEL OPTICAL ARCHITECTURES FOR MICROVOLUME LASER-SCANNING CYTOMETERS (57) Abstract <p>Methods and instrumentation for performing charge coupled device (CCD)-based confocal spectroscopy with a laser spot array are provided. The methods and instruments of the invention are useful in any spectroscopic application, including, but not limited to, microscopy and microvolume laser scanning cytometry (MLSC).</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

NOVEL OPTICAL ARCHITECTURES FOR MICROVOLUME
LASER-SCANNING CYTOMETERS

Background of the Invention

5 Microvolume laser scanning cytometry (MLSC) is a method for analyzing the expression of biological markers in a biological fluid. See, e.g., U.S. Patent Nos. 5,547,849 and 5,556,764; Dietz *et al.*, Cytometry 23:177-186 (1996); U.S. Provisional Application 60/144,798, filed July 21, 1999, each of which is incorporated herein by reference. A sample, such as blood, is incubated in a capillary with one or more
10 fluorescently-labeled probes that specifically binds to particular biological markers, such as membrane proteins displayed on the surface of a blood cell. The sample is then analyzed by a MLSC instrument, which scans excitation light from a laser over the sample along one axis of the capillary, while the capillary itself is moved in an orthogonal axis by an automated stage. Fluorescent probes in the sample emit Stokes-shifted light in
15 response to the excitation light, and this light is collected by the cytometer and used to form an image of the sample. In such images, the cells or particles that bind to the fluorescent probes can be identified and quantitated by image analysis algorithms. The resulting information on the expression of biological markers in the sample can be used for diagnostic and prognostic medical purposes.

20 Current laser scanning cytometers are based on the flying spot confocal laser scanner. These systems scan a laser excitation light spot in one dimension across the sample using a rotating or reciprocating mirror, such as a mirror mounted on a galvanometer. The sample is translated in a direction orthogonal to the scan direction. The collimated excitation laser light follows an epi-illumination path through the
25 microscope objective and is focused on the sample and the mirror scan center is imaged upon the entrance pupil of the microscope objective. Emitted light from the sample is then collected by the microscope objective, and re-traces the excitation light path back to the scanning mirror where it is descanned. The emitted light passes through a dichroic filter and a long-pass filter to separate out reflected excitation light, and is then focussed
30 onto an optical detector through an aperture. The aperture serves as a spatial filter, and reduces the amount of out-of-focus light that is introduced into the detector. The wider the aperture, the greater the depth of focus of the system. The detector generates a signal that is proportional to the intensity of the incident light. Thus, as the laser scans the

sample, an image is assembled pixel-by-pixel. This optical architecture is typically referred to as confocal fluorescence detection.

In order to detect multiple fluorescence probes, the laser scanning cytometry system can also include dichroic filters that separate the emitted light into its component wavelengths. Each distinct wavelength is imaged onto a separate detector through a separate aperture. In this way, an image of the sample is assembled pixel-by-pixel for each emitted wavelength. The individual images are termed channels, and the final multi-color image is obtained by merging the individual channels.

The use of confocal 4-channel fluorescence detection for MLSC is illustrated schematically in FIGURE 1, and is described in the United States Provisional Patent Application entitled "Improved System for Microvolume Laser Scanning Cytometry", filed July 21, 1999, incorporated herein by reference in its entirety and attached hereto as Appendix A. In this embodiment, the light from a laser is scanned over a capillary array wherein each capillary contains a sample that contains fluorescently-labeled species. Specifically, collimated excitation light is provided by a He-Ne laser. The collimated laser light is deflected by an excitation dichroic filter. Upon reflection, the light is incident on a galvanometer-driven scan mirror. The scan mirror can be rapidly oscillated over a fixed range of angles by the galvanometer e.g. +/- 2.5 degrees. The scanning mirror reflects the incident light into two relay lenses that image the scan mirror onto the entrance pupil of the microscope objective. This optical configuration converts a specific scanned angle at the mirror to a specific field position at the focus of the microscope objective. The angular sweep is typically chosen to result in a 1mm scan width at the objective's focus. The relationship between the scan angle and the field position is essentially linear in this configuration and over this range of angles. Furthermore the microscope objective focuses the incoming collimated beam to a spot at the objective's focus plane. The spot diameter, which sets the optical resolution, is determined by the diameter of the collimated beam and the focal length of the objective. Fluorescence samples placed in a capillary array in the path of the swept excitation beam emit stokes-shifted light. This light is collected by the objective and collimated. This collimated light emerges from the two relay lenses still collimated and impinges upon the scan mirror which reflects and descans it. The stokes-shifted light then passes through an excitation dichroic filter (most excitation light reflected within the optics to this point is reflected by

this dichroic) and then through long pass filter 1 that further serves to filter out any reflected excitation light. Fluorescence dichroic filter 1 then divides the two bluest fluorescence colors from the two reddest. The two bluest colors are then focussed onto aperture 1 in order to significantly reduce any out-of-focus fluorescence signal. After passing through the aperture, fluorescence dichroic 2 further separates the individual blue colors from one another. The individual blue colors are then parsed to two separate photomultipliers 1 and 2. The two reddest colors are focused onto aperture 2 after being divided from the two bluest colors by fluorescence dichroic 1. After passing through aperture 2, the reddest colors are separated from one another by fluorescence dichroic 3. The individual red colors are then parsed to photomultipliers 3 and 4. In this way, four separate fluorescence signals can be simultaneously transmitted from the sample held in the capillary to individual photomultiplier light detectors (PMT1-4). Each photomultiplier generates an electronic current in response to the incoming fluorescence photon flux. These individual currents are converted to separate voltages by one or more preamplifiers in the detection electronics. The voltages are sampled at regular intervals by an analog to digital converter in order to determine pixel intensity values for the scanned image.

Other ways are known in the art for obtaining multi-channel information in the microscopy context. For example, it is known in the art to use fluorophores that emit light with overlapping emission spectra but with different time constants of emission. Time-resolved microscopy systems typically use very fast laser pulses and high speed detection circuitry to resolve, in the time-domain, the nanosecond-scale time signatures of the fluorophores. Alternatively, the measurement can be accomplished in the frequency domain with amplitude-modulated laser sources and detection circuitry that measures phase shift and modulation amplitudes. Both of these techniques add significant complexity to the fluorescent measurement system.

Typical MLSC instruments use photomultiplier tubes (PMTs) as light detectors. PMTs are cost-effective and have high data read-out rates which allow the sample to be scanned swiftly. However, a major drawback of the PMT is its low quantum efficiency. For example, in the red to near infrared region of the electromagnetic spectrum, PMTs have quantum efficiencies of less than 10%, *i.e.*, less than one photon in ten that impacts the PMT is actually detected.

In order to have high sensitivity and high measurement speed, it is desirable to use high power laser sources. For each fluorophore, there is a proportional relationship between the intensity of the excitation illumination and the intensity of the emitted light. This proportionality only applies up to the point at which the fluorophore is saturated. At
5 this point, the ground state of the fluorophore is essentially depleted, and all fluorophores exist in the excited electronic configuration. Increasing laser power beyond the saturation point does not increase the intensity of the emitted light. This effect is especially pronounced with fluorophores that have long fluorescent lifetimes, such as inorganic fluorophores, and for quantum dot nanocrystals. These molecules saturate at relatively
10 low power densities because of their long time constants of fluorescence emission. Other undesired processes can occur at higher laser power, including photodestruction and intersystem crossing. In many applications, it is desirable to operate at power densities somewhat below saturation.

In an attempt to increase the speed with which confocal images can be acquired,
15 microscope systems have been developed in which a continuous line of laser excitation light is scanned across the sample, rather than a single spot. The line of emitted light that is produced by the sample in response to the excitation is imaged onto a slit shaped aperture. Since light is distributed over a line of pixels speed limitations due to fluorophore photo-physics are avoided. However, the depth of field, or change in lateral
20 resolution with focus depth, of the line scanner is inversely proportional to the numerical aperture of the objective. MLSC applications require a large depth of field to accurately image cells in a deep blood suspension. High sensitivity and speed require a high numerical aperture lens but would result in a prohibitively small depth of field. This tradeoff ultimately results in limited speed and sensitivity.

25 Given the limitations using a PMT as a light detector, much research is currently directed towards developing higher efficiency detectors that will allow rapid image acquisition at below-saturation power densities. One such light detector is the charge coupled device (CCD). See, e.g., G. Holst, CCD Arrays, Camera and Displays, 2d Ed., JCD Publishing and SPIE Optical Engineering Press 1998. The CCD consists of an
30 interlinked array of sensitive photodetectors, each of which can have a quantum efficiency of greater than 80%. Despite their high efficiency, CCDs are not ideal for use in the MLSC context. One reason is that the CCD is usually employed as an imaging device in

which the entire field of view is excited and the CCD captures all of the emitted light in the field of view. Used in this way the depth of field and sensitivity are coupled just as in a line scanner. Furthermore, the full field illumination and collection means a substantial amount out of focus light is excited and received by the CCD detector. Even if a CCD is used in non-imaging mode in combination with a scanned laser spot and a pinhole aperture--much in the same way as a PMT is used--additional problems are encountered. Firstly, when replacing PMTs with CCDs for simultaneous multi-channel image acquisition, a separate CCD is required for each channel. The cost of providing a separate high-efficiency CCD for each channel adds greatly to the cost of the instrument.

Moreover, CCDs take significantly longer to read out than PMTs, thereby placing a significant limitation on the speed with which data can be acquired.

The present invention is directed towards optical architectures for spectroscopy which can acquire data with greater speed than prior art systems. The instruments of the invention can also be used for time resolved measurements of fluorophore emission. The methods and instruments of the invention are useful in any application where spectroscopic data from a sample is required. In preferred embodiments, the methods and instruments of the invention are used for MLSC.

The invention uses CCDs in which binning is used to subdivide a single CCD into pixel groupings that collect data simultaneously from a number of different regions of a sample. Preferred embodiments of the invention use multiple laser excitation spots in combination with CCD light detectors. In some embodiments, the individual bins are further subdivided to provide spectral information for each region of the sample. The pixel intensity values for each bin are assembled by computer to give seamless images of the sample in each channel.

Summary of the Invention

Two issues typically limit the speed and sensitivity performance of prior art systems. Firstly, commonly used PMT detectors have low quantum efficiencies, especially in the red to near infrared region of the optical spectrum. Secondly, these systems typically scan a focused laser spot to excite fluorescent emission in the sample. For high sensitivity and measurement speed, it is desirable to use a high power density excitation source. However, beyond certain saturating power densities (power per unit

area of the laser spot), the excitation source saturates the fluorescent labels, preventing further improvement in sensitivity and measurement speed.

The preferred embodiment of the present invention uses CCD detectors (instead of PMTs) as non-imaging light-detecting devices in a confocal scanning architecture, where
5 an array of laser spots is scanned across the sample, instead of a single spot. Two features of this invention solve the limitations described above. Firstly, the high power laser excitation is divided into multiple spots, thus reducing the power density in each spot and minimizing sensitivity and laser power limitations due to fluorophore saturation. Secondly, the CCD is used in a non-imaging mode, by defining multiple effective
10 confocal apertures as "binned" regions of pixels on the 2 dimensional surface of the device. Each binned region is matched to an excitation laser spot which is focused into the sample. This architecture retains the controllable depth of field of a PMT-based confocal spot scanner, but also takes advantage of the very high quantum efficiencies available with CCD detectors.

15

Brief Description of the Drawings

Note, that in all the drawings, the optical pathways are illustrated schematically. Angles and dimensions are not to scale.

20 FIGURE 1 illustrates a single-spot multi-channel MLSC system in which mechanical confocal apertures and photomultipliers are used. The chief ray of each ray bundle is traced.

FIGURE 2 illustrates a 2-channel spectroscopy system in which a sample is scanned with 3 laser excitation spots, and the resulting emission light is imaged onto CCD
25 light detectors that have been partitioned into three confocal bins. The chief ray of each ray bundle is traced.

FIGURE 3 illustrates a 512 x 64 pixel CCD detector that is partitioned into three rectangular confocal bins.

FIGURE 4 illustrates the relative motion of three laser excitation spots as they are
30 scanned over a moving sample.

FIGURE 5 illustrates one embodiment for performing multispot, multichannel confocal spectroscopy using a single CCD and a confocal slit aperture. The chief ray of each ray bundle is traced.

FIGURE 6 illustrates schematically a 625 pixels x 488 pixels CCD light detector
5 that has been configured for a 6 spot system with 4 spectral channels.

FIGURE 7 illustrates a time-resolved confocal spectroscopy system in which a binned CCD collects the emission light at predetermined times following laser spot excitation.

FIGURE 8 illustrates a time-resolved confocal spectroscopy system in which
10 multiple optical fibers act as confocal apertures that are imaged over the sample at predetermined times after laser spot excitation.

FIGURE 9 illustrates schematically a non epi-illuminated spot scanner system.

Detailed Description of the Preferred Embodiments

15 The present invention provides spectroscopy methods and instrumentation with a number of novel optical configurations that allow multichannel images to be acquired quickly, and/or with time-resolution of the individual fluorophore emissions. In preferred embodiments, the invention uses CCDs as light detectors, wherein groups of pixels on the CCD form bins that are imaged onto the sample by the scanning optics. In preferred
20 embodiments, each bin functions as a confocal aperture. The size of the bin determines the width of the cone of emitted light that is detected, and hence the greater the bin size, the greater the depth of field. Light that falls on the CCD outside of the bin is not detected. Hence, each bin functions in the same way as a mechanical confocal aperture. In preferred embodiments, the invention uses an array of laser spots to scan the sample
25 simultaneously in multiple locations. Emitted light from each spot is imaged onto a separate confocal CCD bin, and the image is built by fusing the separate images from each spot together. In other embodiments, a series of bins are imaged onto the sample at different times following excitation such that each bin on the CCD represents a different emission time, thereby enabling time-resolved fluorescence measurements to be made.
30 The advantage of using CCD bins as confocal apertures is that re-configuration of the instrument is performed simply by changing the size and position of the bins on the CCD, rather than by any mechanical operation. The advantage of using multiple spots is that

lower laser power is present at each spot in comparison to a single spot system. The lower laser power density minimizes fluorophore saturation, but total system throughput is maintained by simultaneously detecting the emission from multiple excitation spots.

Note, that in all the embodiments that follow, the methods and instrumentation of the instant invention are described in the context of MLSC. Those of skill in the art will understand, however, that the methods and instruments of the invention are useful in any spectroscopy or cytometry application, including microscopy applications. In addition, although a fluorescence imaging application is described, this scanning system can be applied to many light scatter detection modes. Examples of such possible modes include: luminescence, phosphorescence, Raman scattering, Rayleigh scattering and Mie scattering.

Multiple laser spot excitation system with binned CCD light detection

In one embodiment of the invention, a laser excitation beam is converted into an array of beams, by a device such as a Damann grating. Alternatively, other spot generating devices may be used, such as a microlens array or a fiber bundle. The system is not limited to the use of a linear array of spots and can function with a two dimensional array of spots. This could allow a greater area of a CCD detector area to be used and thus enhance readout performance. Other embodiments of the device might not use a single laser beam excitation source, but rather a laser diode array, thereby omitting the requirement for a separate beam generator device. The source of the beam is imaged, with relay lenses, onto the center of the scanning mirror device, such as a galvanometer. Other embodiments of the present device include the use of other beam deflection methods. Such methods include, but are not limited to, a piezoelectric scanner, polygonal mirrors, acousto-optic deflectors, and hologons. In the present embodiment, the scan center of the galvanometer is in turn imaged by a second set of relay lenses into the entrance pupil of a microscope objective. The laser beam array is thus focused by the objective into an array of spots in the focal plane of the objective. Each spot in the array scans and excites a separate region of a sample, which sample is moved at constant velocity along the axis orthogonal to the laser spot scan axis. Fluorescent light that is emitted by the sample is collected by the objective lens, passes through a dichroic filter and is imaged onto the surface of a CCD detector that has been electronically divided into a bin of pixels of the

desired size. Emitted light that impinges the CCD outside of the bin is not detected; hence the bin functions as a confocal aperture in which the confocal depth of focus can be controlled simply by changing the bin dimensions. The greater the area of the bin, the greater the depth of focus.

5 The multi-spot system can be used for multichannel imaging by dividing the fluorescent emission into individual wavelengths--using, for example, dichroic filters--and then directing each component wavelength to a separate CCD detector. In this embodiment, a different CCD is used for each channel, but the bin configuration for each CCD is identical. The CCDs are periodically read out in synchrony to maintain proper
10 registration of the individual color images. Hence, this embodiment provides a multichannel MLSC instrument in which the confocal depth of focus is computer-controlled (by changing the bin dimensions), rather than being mechanically-controlled (by changing the size of a confocal aperture).

FIGURE 2 illustrates one embodiment of the invention where 3 laser excitation
15 spots are generated, then reflected off an excitation dichroic onto a galvanometer scan mirror. (In this figure 3 spots are chosen to illustrate the invention for convenience sake. As described below, the present invention includes any system with more than one spot.) The scanning spots pass through relay lenses to the entrance pupil of a microscope objective, and are focussed onto the sample. Emission light from the sample (three
20 emission rays) is collected by the microscope objective, and retraces the path of the excitation spots back to the dichroic filter. The emission light passes through the excitation dichroic and a long-pass filter, and is separated into two wavelength portions by an emission dichroic filter. The two portions are then imaged by a focus lens onto separate CCDs, wherein each CCD is partitioned into three confocal bins. A schematic illustration
25 of a 512 x 64 pixel CCD detector that is partitioned into three rectangular confocal bins is provided in FIGURE 3.

In preferred embodiments, the linear array of laser spots excites emission from the sample. The scanning mirror device rotates scanning the laser spots in the direction that is parallel to the line defined by the array of spots. The total scan deflection of each
30 spot is chosen such that each spot scans across a length of the sample that is approximately the same length as the distance between the spots. The sample is moved

along the orthogonal axis to the laser spot scan axis. This is illustrated schematically in FIGURE 4A, where three spots scan in the vertical axis and the sample is moved horizontally. Hence, the relative spot motion traces a sawtooth pattern. As the spot array is scanned across the sample by the scanning mirror device, the CCD bins are periodically read out. The timing of this read out operation determines the pixel size in the scan dimension. Alternatively (FIGURE 4B), the three spots are arrayed parallel to the sample movement. The spots are scanned across the complete sample. When one spot reaches the start scan position of the next spot, the sample is shuttled so that the first spot starts scanning again at the previous stop position of the last spot.

As the scan proceeds, each laser spot generates a 2-D image that is acquired by the corresponding bin of the CCD detector. The images from each spot either do not overlap, or overlap only slightly. When the scan is complete, the individual images can be joined together by a computer to provide a single seamless image.

Any number of spots can be used in the instant invention. The advantage of using multiple spots is that lower laser power density is applied to each spot, minimizing fluorophore saturation. For example, each spot in a 10 spot array has $1/10^{\text{th}}$ the power density of the laser spot in a single spot system using laser sources of equal power. However, each spot dwells 10 times longer in any region of the sample than the single spot system, so that the total photon flux per image pixel is the same. Since all 10 spots are excited and detected in parallel, the total scan time for a sample is the same in either case. However, by using CCDs as light detectors, significant enhancements in sensitivity result. A CCD can have at least 3 times greater quantum efficiency as a PMT; moreover using a lower excitation power density can give a significant increase in sensitivity due to the avoidance of saturation, photo-destruction and other nonlinear process excitation. Thus, the multispot system with CCD detection can be 6 to 10 times more sensitive than a single spot PMT system operating at the same scan speed. This increased sensitivity can be exploited to shorten the scan time, so a multispot system can yield comparable images to a single spot system, but in significantly less time. Alternatively, the multispot CCD system can operate at the same scan rate as the single spot system, but will be able to detect emission intensities that a conventional PMT single spot system could not detect at that scan rate. An even further advantage of using low laser power densities is that it

allows the use of fluorophores that saturate at comparatively low power densities, such as inorganic fluorophores or quantum dot nanocrystals with long emission time constants.

The limit on the number of spots is determined by the required axial response of the system and the amount of cross talk between spots that can be tolerated. The more spots in the array, the more closely spaced are the confocal bins on the CCD. Axial response is proportional to bin size and so will be effectively reduced. Furthermore, the closer bins means light rejected from one bin will impinge upon another ultimately reducing system sensitivity. The present invention includes any system with more than one spot. Preferably there will be between 2 and 1000 spots and more preferably between 5 and 400.

Using CCD bins as confocal apertures is a substantial advance due to the relative simplicity of changing the dimensions of the confocal depth of field. Mechanical confocal apertures in focused light systems are typically only several μm in diameter, and so require sophisticated and precise mechanical systems to control the aperture size. By contrast, a CCD bin can be changed simply by reconfiguring the CCD array using a computer.

The use of a CCD in MLSC is a significant improvement over prior art MLSC instruments that use PMT for light detection. The biological fluids that are assayed by MLSC auto-fluoresce and can absorb or scatter excitation light. The use of fluorophores that are excited by red light (such as the 633nm line from a HeNe laser) reduces these problems and allows MLSC assays to be performed in whole blood. However, PMTs have a quantum efficiency of less than 10% in the red portion of the electromagnetic spectrum, leading to poor sensitivity when these fluorophores are used. By contrast, many types of CCDs have quantum efficiencies of greater than 80% in the same region of the spectrum.

As mentioned previously, current CCD detectors have a lower data read-out rate than PMTs. If a single spot is scanned over a sample and the emitted light imaged onto a CCD, the CCD would have to be read out sequentially for every single pixel in the image. By contrast, the multispot system provided by the instant invention can simultaneously acquire data for X pixels, where X is the number of spots. Thus, a 10 spot system provides data for 10 pixels in the image at each read-out event, whereas a single-spot system provides data for just a single pixel at each read-out event. Hence, the multispot

system of the instant invention allows the benefits of enhanced sensitivity provided by the CCD to be achieved while minimizing the problems associated with the low data read out rate of CCDs. CCDs with higher read out rates will likely be available in the future.

Using such improved CCDs will further increase the sensitivity and speed of the

5 instruments and methods of the instant invention.

Note that all of the embodiments of the present invention can use conventional PMTs as the light detectors, rather than CCDs. In these embodiments, conventional confocal apertures are required to give the required rejection of out of focus fluorescence. The apertures would be arranged in a pattern identical to the laser spot array.

10

Multiple laser spot excitation system with spectral analysis on a single CCD

In certain embodiments, a single CCD is used for multichannel imaging of a sample. In these embodiments, a line of laser spots is scanned over the sample, and emitted light is imaged, as described above, onto a line of confocal apertures. The layout
15 of the array of apertures parallels the layout of the array of laser spots, such that the emitted light from each laser spot passes through a different aperture. After passing through the aperture, each beam of emitted light may be passed through dispersal optics that spread out the component wavelengths. Suitable wavelength dispersing optics include, but are not limited to, echelle gratings, holographic concave gratings,
20 transmission gratings, or prisms. In addition, particular wavelengths can be directed mechanically onto the detector with the use of a constant deviation dispersion prism, such as the Pellin-Broca prism, or through the use of a resonant grating filter. Electro-optic methods to select wavelengths include the use of an acoustic-optic tunable filter or electro-optic resonant grating filter. The dispersal optics also image each aperture onto a separate
25 rectangular region of a CCD so that the light that passes through each aperture is spectrally-spread along the long axis of a single rectangle. Each rectangular region on the single CCD is subdivided into bins along its long axis so that each bin collects a different wavelength of the spread light. For example, for 4-color fluorescent detection, each rectangle can be subdivided into 4 spectral bins along its long axis. Hence, each
30 rectangular region on the CCD can essentially perform spectral analysis of the light emitted in response to excitation by a particular spot.

In a preferred system for this embodiment, the sample is scanned with a line of laser spots, and all the emitted light from the sample is imaged onto a single rectangular "slit" confocal aperture that is parallel to the line of laser spots. The emitted light then passes into dispersal optics that spectrally-spread each emitted light beam into its component
5 wavelengths. The axis of dispersion is orthogonal to the long axis of the confocal "slit". The dispersal optics also image the component wavelengths from each emission spot onto a separate rectangular CCD region, wherein the long axis of each CCD rectangle is parallel to the axis along which the dispersal optics spread the emission spot. Consequently, the long axis of each CCD rectangle is orthogonal to the long axis of the
10 "slit" aperture. Each rectangular region is subdivided along its long axis into spectral bins such that each of the spectral bins collects a different wavelength of light resulting from the dispersal of a single emission spot. The rectangular regions of the CCD function as a second "slit" confocal aperture oriented in the opposite dimension to the mechanical "slit" aperture. As a result, the final image is confocal in both dimensions. The depth of focus
15 in this system can be controlled by coordinately varying the width of the mechanical "slit" aperture and the width of each CCD rectangle.

FIGURE 5 illustrates schematically one embodiment using a slit aperture and a concave grating for wavelength dispersal. In this illustration, laser light is reflected onto the spot generating optics -by mirror-. Three laser spots are generated by spot generating
20 optics, passed by lenses 1 and 2 to a dichroic filter, which dichroic reflects the laser spots on a scanning galvanometer mirror. The spots are then passed by lenses 3 and 4 to mirror 2, so they re-converge at the entrance pupil of the microscope objective. The objective focuses the spots onto the sample and the light emitted from the three spots is collected by the objective. The emission light rays re-trace the path of the laser spots to the dichroic
25 filter. The emission light passes through the dichroic, followed by lens 5 which focuses the light at the slit aperture. The focused light passes through a long pass filter, and then through a confocal slit aperture that is oriented with the long axis of the slit parallel to the vertical axis. Emission light rays that pass through the slit aperture then fall on a concave grating that re-images the spots and wavelengths onto the detector. In this illustration,
30 each emission light ray is spread into multiple wavelengths along the horizontal axis. Thus, the horizontal axis of the CCD provides spectral information about each emitted light ray, and the vertical axis provides spatial information.

FIGURE 6 illustrates schematically a 625 pixels x 488 pixels CCD light detector that has been configured for a 6 spot system with 4 spectral channels. The CCD is divided into 6 rectangular regions, and each region is subdivided into 4 spectral bins. As in
5 axis provides spatial information when used in combination with a vertically-oriented confocal slit aperture. The height of each rectangle in FIGURE 6 can be adjusted to vary the confocality of the image in the horizontal axis. A suitable CCD for this application is the Pluto™ CCD from Pixelvision.

As described above, previous attempts to use line illumination in MLSC have not
10 yielded the desired speed and sensitivity improvement because of the interaction of collection numerical aperture and system depth of field. The instant invention provides for the first time a method for distributing excitation light over an area larger than a single spot while maintaining the depth of field and axial response of a single flying spot confocal laser scanner. This is accomplished by: a) scanning the sample with individual
15 spots of excitation light rather than a continuous line of light; and b) using a CCD bin confocal apertures, with each bin corresponding to an excitation spot.

This embodiment is also mechanically simpler than the embodiment above in which a line of pinhole apertures is used. Changing the size and orientation of a single slit aperture is simpler than changing the size of a series of comparatively smaller pinhole
20 apertures. Thus, this embodiment retains the true two-dimensional confocality of the pinhole aperture architecture, while also possessing the mechanical simplicity of the confocal slit architecture.

An additional advantage of performing spectral analysis on the CCD in the manner outlined above is that the CCD binning in the spectral dimension can be controlled
25 electronically. Each detection color can be optimized for the specific assay that is to be performed. This also eliminates the need in the detection system for many dichroic filters, which can vary from unit-to-unit and with temperature and humidity.

An even further advantage of using the CCD systems outlined above is that alignment of the mechanical confocal apertures with the CCD can be easily accomplished
30 electronically. Rather than physically moving the apertures, the position of the bins on the CCD can be adjusted in order to insure that each bin is in perfect registration with its

corresponding aperture. This process can be automated using, for example, a test slide containing all the fluorescent labels that are to be used in the assay.

In further embodiments of this invention, it is possible to use non epi-illumination of the sample. In this embodiment, illustrated in FIGURE 9, the excitation light is brought
5 to the sample without passing through the collection objective. This method is referred to as off-axis illumination. See, e.g., U.S. Patent No. 5,578,832. As in epi-illumination a fan of laser beams is generated. Possible generating optics include but are not limited to Damann and other gratings, fiber optic bundles, micro-mirror arrays, acousto-optic and electro-optic devices. The fan of rays are collected by the first fan lens and re-converged
10 on a scanning device such as a reciprocating mirror with a second fan lens. The rays then pass through a final lens such that each spot is focused on the sample. The final lens is configured such that the excitation beams are at approximately 45 degrees to the sample. Emitted light is then collected and re-imaged on the CCD detector with a tube lens. Unwanted excitation light is eliminated with a long pass blocking filter. If the spots are
15 not de-scanned then the scanned spots will move on the detector, however the correct CCD bins can be chosen so that the readout follows the spots. Alternatively, the collected rays can pass via a second reciprocating device such as a mirror, in sync with the excitation mirror, to de-scan the spots. A number of different array detectors can be used to collect discrete wavelengths where the wavelengths are selected by optical filters, e.g. a
20 dichroic filter. As in epi-illumination a dispersive element can be used to spread wavelengths over the array detector orthogonal to the spots.

Despite the extra complications involved in de-scanning the spots, off-axis has some advantages over epi-illumination. No excitation dichroic filter is needed and so many different excitation wavelengths can be used without having to change filters.
25 Furthermore, extreme excitation wavelengths, i.e. ultraviolet or infrared, that are incompatible with collection optics can be used. Examples of reporters that use these wavelengths are: 2 photon up converting phosphors that use 980nm excitation and emit in the visible region; and nano-crystals that are optimally excited in the UV, < 400nm, but emit in the visible regions. See, e.g., Bruchez *et al.*, Science 281:2013 (1998); Wright,
30 W.H. *et al.*, Proceedings of SPIE – The International Society for Optical Engineering Ultrasensitive Biochemical Diagnostics II Feb 10-Feb 12 97 v 2985 1997 San Jose, CA, USA.

All embodiments of the invention described above include system designs where the regions of the sample illuminated by the spot array are imaged by an optical system onto the surface of a CCD detector. Alternative system embodiments use mechanical apertures to provide the necessary confocal apertures, with non-imaging optical systems, such as fiber optics or fiber bundles, to transfer light passed through the apertures to the surface of the detector. Thus the system designer can choose the optimal spatial mappings between the excitation spot array and the detector surface. This allows the designer to choose from a wider variety of detector devices, or to more efficiently utilize the surface area of the device. For example, if the excitation spot array consists of a linear array of spots, a linear array of apertures could be used to collect the emitted light from the sample passing the light into optical fibers, with one fiber or fiber bundle per aperture. The outputs of the multiple fibers or fiber bundles could be arranged, for example, into a square-shaped 2-dimensional array, and imaged, directly or through dispersing optics, onto the surface of the detector. In this manner the designer can provide a better match to the form factor of a given CCD device, or fill up the surface of a CCD with more spots than could be utilized with imaging optics only.

Time-resolved spectroscopy systems

The methods of the present invention can also be used to perform time-resolved MLSC. As described above, in time-resolved fluorescence microscopy, images of the sample are taken at predetermined time intervals after excitation illumination. This allows observation of multiple fluorophores with different emission time constants. In the present invention, time-resolved images can be obtained by imaging a series of confocal CCD bin apertures over the sample at predetermined times behind the laser excitation spot(s). The confocal bins are scanned over the sample by the same optical system that scans the laser spot. The physical separation between CCD bins maps into a difference in emission time for the sample. The time separation is a function of the scan velocity across the sample.

Such a system can function as follows in one embodiment illustrated schematically in FIGURE 7. At $t=0$, the laser spot excites a first region of the sample in which fluorophore F1 and F2 are present. F1 has an emission time constant such that the fluorescence emitted from F1 is practically coincident with excitation. Hence, light from F1 retraces the path of the laser beam, passes through a dichroic filter, and is imaged onto CCD bin

B1. At $t=1$, the scanning mirror has deflected, and a second region of the sample is receiving excitation illumination. Also at $t=1$, F2 which was excited in the first region of the sample at $t=0$ emits. Because the scan mirror has deflected between $t=0$ and $t=1$, the light path followed by F2 emission is not coincident with the laser path. As a result, the fluorescence from F2 follows a path that is displaced by a predetermined amount relative to fluorescence from F1. Light from F2 can be collected by a separate confocal bin, B2, on the CCD. It will be understood that additional bins can be defined on the CCD in order to obtain additional time intervals. The distance between the bins (at constant scan speed) determines the time interval between each fluorescence measurement event.

In other embodiments, a multispot excitation array as described above is used for time resolved measurements. In this embodiment, the CCD is divided into a matrix of bins. In one dimension, the bins provide positional information for the emitted light. In the other dimension, the bins provide time-resolved fluorescence measurements. For example, a system for performing three time-resolved measurements for each 10 excitation laser spots would comprise a 10×3 array of CCD bins. The dimensions of each bin can be independently varied in order to optimize detection for particular fluorophores.

In other embodiments, time-resolved spectroscopy is performed using multiple pinhole confocal apertures operatively coupled to light detection devices. The spacing between the confocal apertures determines the time intervals for the fluorescence measurement events. As in the embodiment involving CCD bins, the individual pinhole confocal apertures are scanned over a particular region of the sample at different times after excitation of that region. As an alternative to pinhole apertures, this embodiment can be performed using optical fibers. The core of each fiber acts as a pinhole, and the light transmitted through the fibers is delivered to multiple PMTs. As before, the spacing between the illuminated end of the optical fibers determines the time interval between each fluorescence measurement. This embodiment is illustrated schematically in FIGURE 8.

In still further embodiments, time resolved fluorescence spectroscopy is performed in tandem with emission wavelength spectroscopy of the light emitted at each time interval. In certain embodiments, this is done using a series of pinhole apertures that are imaged over the sample as described above at different times behind a single laser excitation spot.

Emission light that passes through each aperture is then passed through dispersal optics--such as a concave diffraction grating or a prism--that spread the emitted light into its component wavelengths. The component wavelengths from each time interval are then imaged by the dispersal optics onto a separate rectangular region of a CCD, wherein the
5 long axis of the rectangle is parallel to the axis along which the emitted light was spread. Each pinhole aperture is mapped to a separate rectangular region on the CCD. The individual rectangles are subdivided along their long axes into spectral bins, and the spread light from each aperture falls onto those bins in a wavelength-dependent manner.

In even further embodiments, the invention provides a method for performing
10 mutispot time-resolved fluorescence spectroscopy in tandem with fluorescence emission wavelength spectroscopy. This system functions in the same way as the mutispot system with a confocal slit architecture, as described above. However, in order to perform time-resolved measurements, the system has a series of slit apertures that are imaged over the sample at time intervals behind the excitation spots. Light passing through each aperture
15 is dispersed into its component wavelengths and imaged onto spectral bins arranged in rectangles on a CCD, wherein the rectangles are orthogonally oriented to the confocal slit. In certain embodiments, separate CCDs are used to image the light coming through each confocal aperture; hence, a three-slit configuration would require three CCDs. In other embodiments, a single CCD is used to image the light from all of the apertures. The CCD
20 in this embodiment would be configured to provide a matrix of rectangles; each aperture is imaged onto a particular row (or column) of rectangles on the CCD. Thus, a single CCD provides data on the position, time-resolution, and spectrum of each fluorescence emission event.

What is claimed is:

1. A confocal scanning system comprising;
 - (a) means for generating and scanning over a sample a plurality of spots of excitation light, whereby emission light is released by said sample in response to excitation by each said spot;
 - (b) one or more detection devices positioned so that said emission light is simultaneously imaged thereupon.
2. The confocal scanning system of claim 1 wherein 3-100 spots are generated.
3. The confocal scanning system of claim 1 wherein 5-25 spots are generated.
4. The confocal scanning system of claim 1 wherein said emission light comprises multiple component wavelengths.
5. The confocal scanning system of claim 4 wherein each said component wavelength is imaged onto a separate detection device by one or more dichroic filters.
6. The confocal scanning system of claim 1 wherein said sample comprises a blood sample contained within a capillary.
7. The confocal scanning system of claim 6 wherein said capillary is translated orthogonal to the scan of excitation light.
8. The confocal scanning system of claim 6 wherein the spots of excitation light are scanned in a direction parallel to the axis said capillary.
9. The confocal scanning system of claim 6 wherein the spots of excitation light are scanned in a direction perpendicular to the axis said capillary.

20

10. The confocal scanning system of claim 1 wherein said one or more detection devices are charge coupled devices (CCD).

11. The confocal scanning system of claim 10 wherein each CCD is partitioned into
5 multiple bins such that each bin collects a portion of the emission light resulting from the excitation of said sample by one of said spots.

12. The confocal scanning system of claim 11 wherein the dimensions of each said bin are selected such that only emission light from within a predetermined focal depth of said
10 sample is collected.

13. The confocal scanning system of claim 4 further comprising means for dispersing emission light into its component wavelengths.

14. The confocal scanning system of claim 13 wherein said means for dispersing
15 emission light into its component wavelengths is a dichroic filter.

15. The confocal scanning system of claim 13 wherein said means for dispersing emission light into its component wavelengths is a prism.

20

16. The confocal scanning system of claim 13 wherein said means for dispersing emission light into its component wavelengths is a grating.

17. The confocal scanning system of claim 13 wherein one detection device is employed.

25

18. The confocal scanning system of claim 17 wherein said detection device is a CCD.

19. The confocal scanning system of claim 1 further comprising a microscope objective.

20. The confocal scanning system of claim 19 wherein said excitation light and said
30 emission light pass through said microscope objective.

21

21. The confocal scanning system of claim 1 further comprising one or more fiber optics to transfer emission light to the one or more detection devices.
22. The confocal scanning system of claim 13 further comprising an aperture
5 corresponding to each spot of emission light so that only emission light from within a predetermined focal depth of said sample passes through to the detection device.
23. The confocal scanning system of claim 11 further comprising a slit aperture
10 corresponding to each spot of emission light so that only emission light from within a predetermined focal depth of said sample passes through to the detection device.
24. A confocal scanning system comprising;
- (a) means for generating and scanning over a sample along an axis a plurality spots of excitation light; whereby emission light is released by said sample in response to
15 excitation by said spots;
- (b) a spatial filter comprising a rectangular aperture, said spatial filter positioned such that said emission light is imaged thereupon;
- (c) means for dispersing emission light that passes through said spatial filter into its component wavelengths; and
- 20 (d) a CCD, said CCD positioned such that said component wavelengths are imaged thereupon;
- wherein said CCD is partitioned into rectangular pixel regions orthogonal to said spatial filter such that each rectangular region receives a portion of the emission light resulting from the excitation of said sample by one of said spots;
- 25 wherein each rectangular region is subdivided along its long axis into at least two spectral bins such that each spectral bin collects a different component wavelength of said portion; and
- wherein the dimensions of each said spectral bin are chosen such that said portion comprises emission light from a predetermined focal depth of said sample.
- 30
25. A system for time-resolved confocal scanning, comprising:

22

- (a) means for generating and scanning over a sample along an axis one or more diffraction-limited spots of excitation light; whereby emission light is released by said sample in response to excitation by said spots;
- (b) a plurality of confocal apertures, each said confocal aperture positioned so that the emission light resulting from excitation of said sample by one of said spots is imaged thereupon by said scanning means at a predetermined time following excitation by said spot;
- (c) means for light detection operatively coupled to said confocal apertures.
- 10 26. The system of claim 25, wherein said means for light detection is a CCD, and wherein said confocal apertures comprise pixel bins on said CCD.
27. A confocal scanning system comprising:
- 15 an excitation energy delivery system to direct energy toward a first region of a sample;
- an optical detection system for measuring fluorescence of the sample induced by the energy;
- a spatial filter disposed optically between the sample and the optical detection system to limit the measured fluorescence to at least one second region of the sample; and
- 20 a mechanism coupling the energy delivery system and the spatial filter to the sample so that the first and second regions scan the sample sequentially.
28. The system of claim 27 wherein the mechanism scans the first and second regions at a speed and with a distance therebetween so that the fluorescence is measured a
- 25 predetermined time after the energy.
29. The system of claim 27 further comprising a plurality of spatial filters, the spatial filters comprising pinhole apertures aligned so that the fluorescence is measured at a plurality of times after the energy.
- 30 30. The system of claim 27 wherein the energy comprises laser energy.

1/9

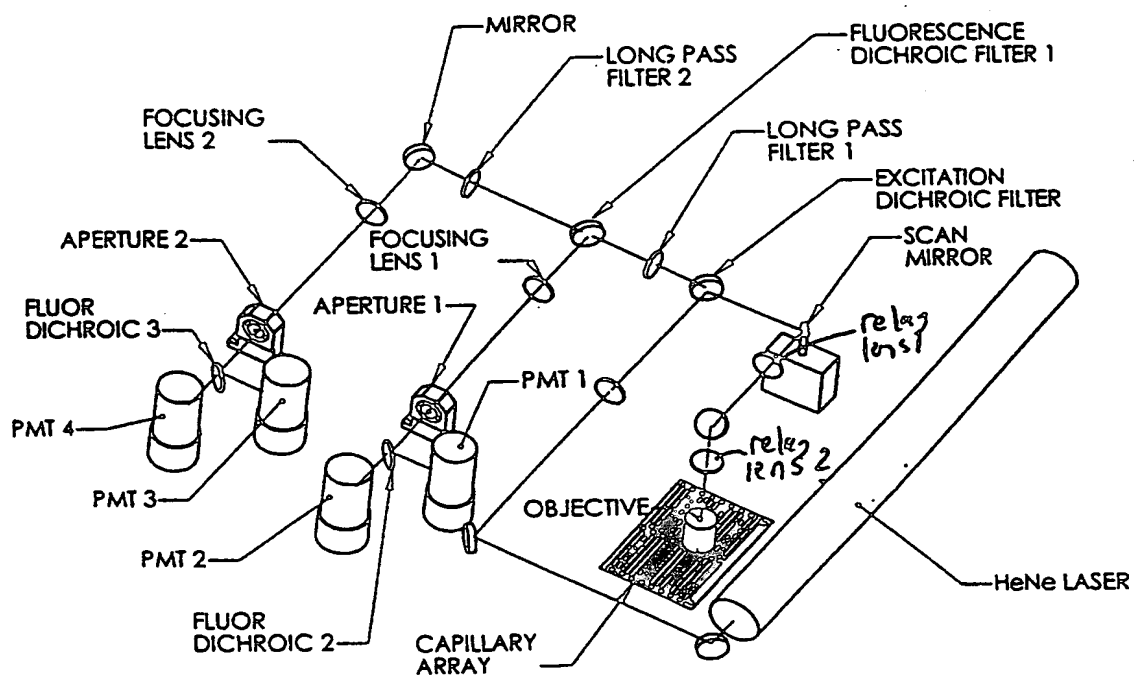


Fig. 1

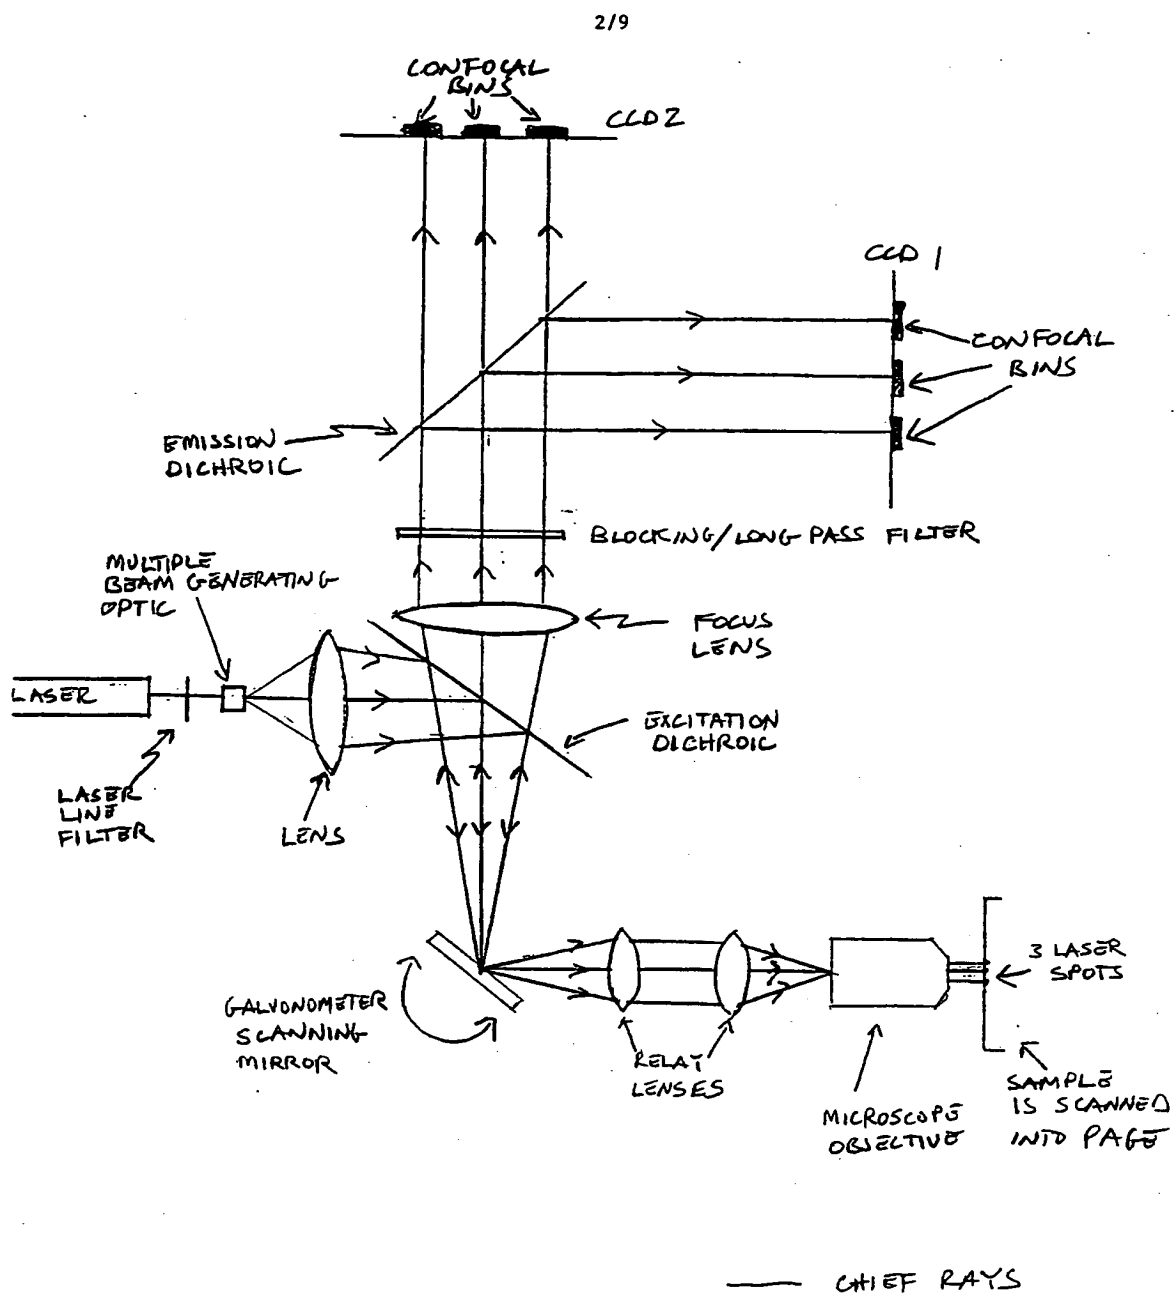


Fig. 2

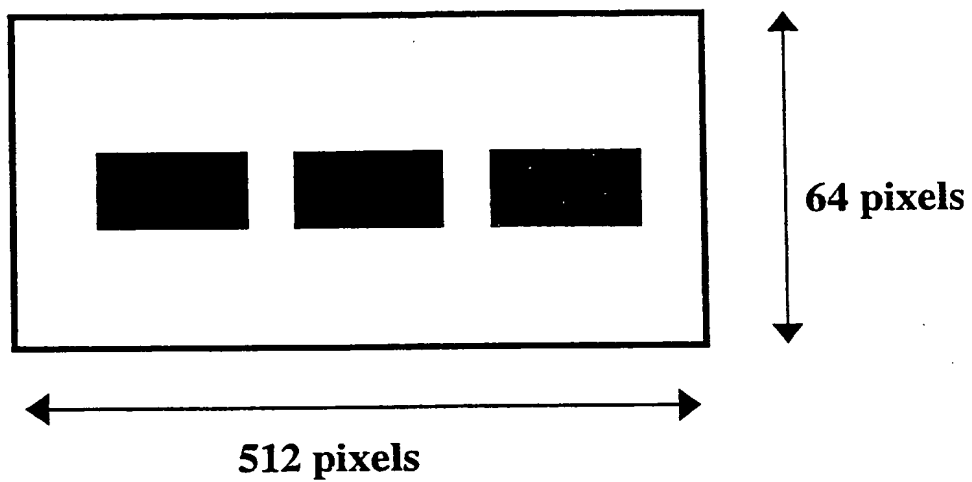


FIGURE 3

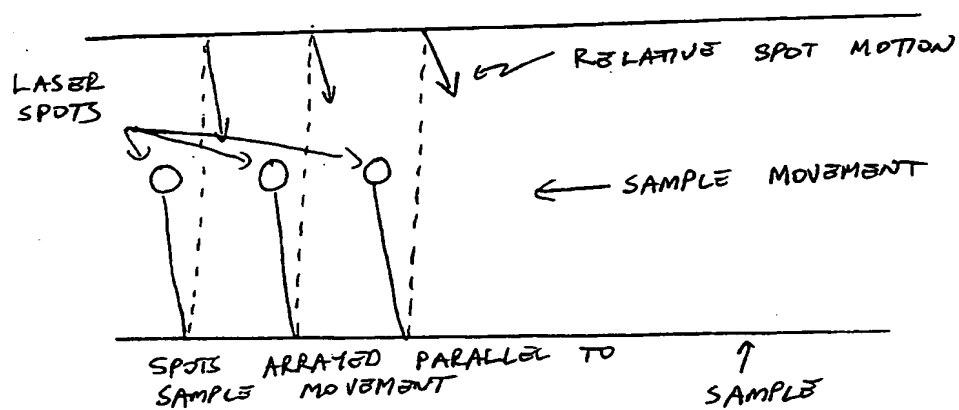


Fig. 4A

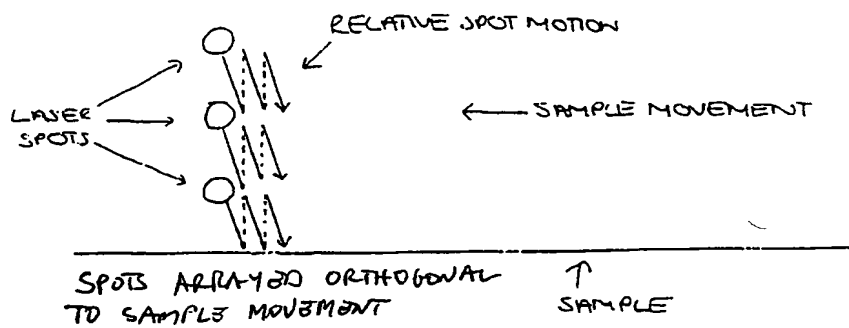


Fig. 4B

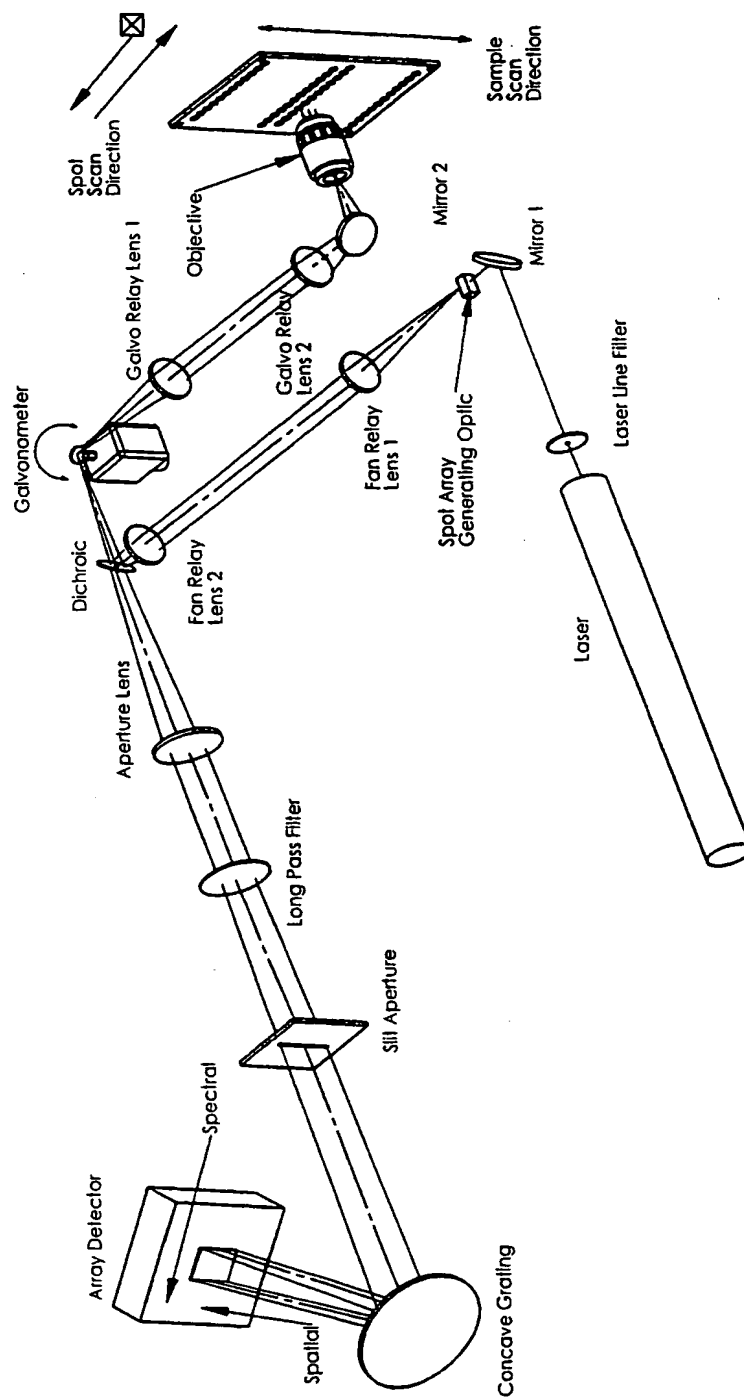


Fig. 5 — CHIEF RAYS

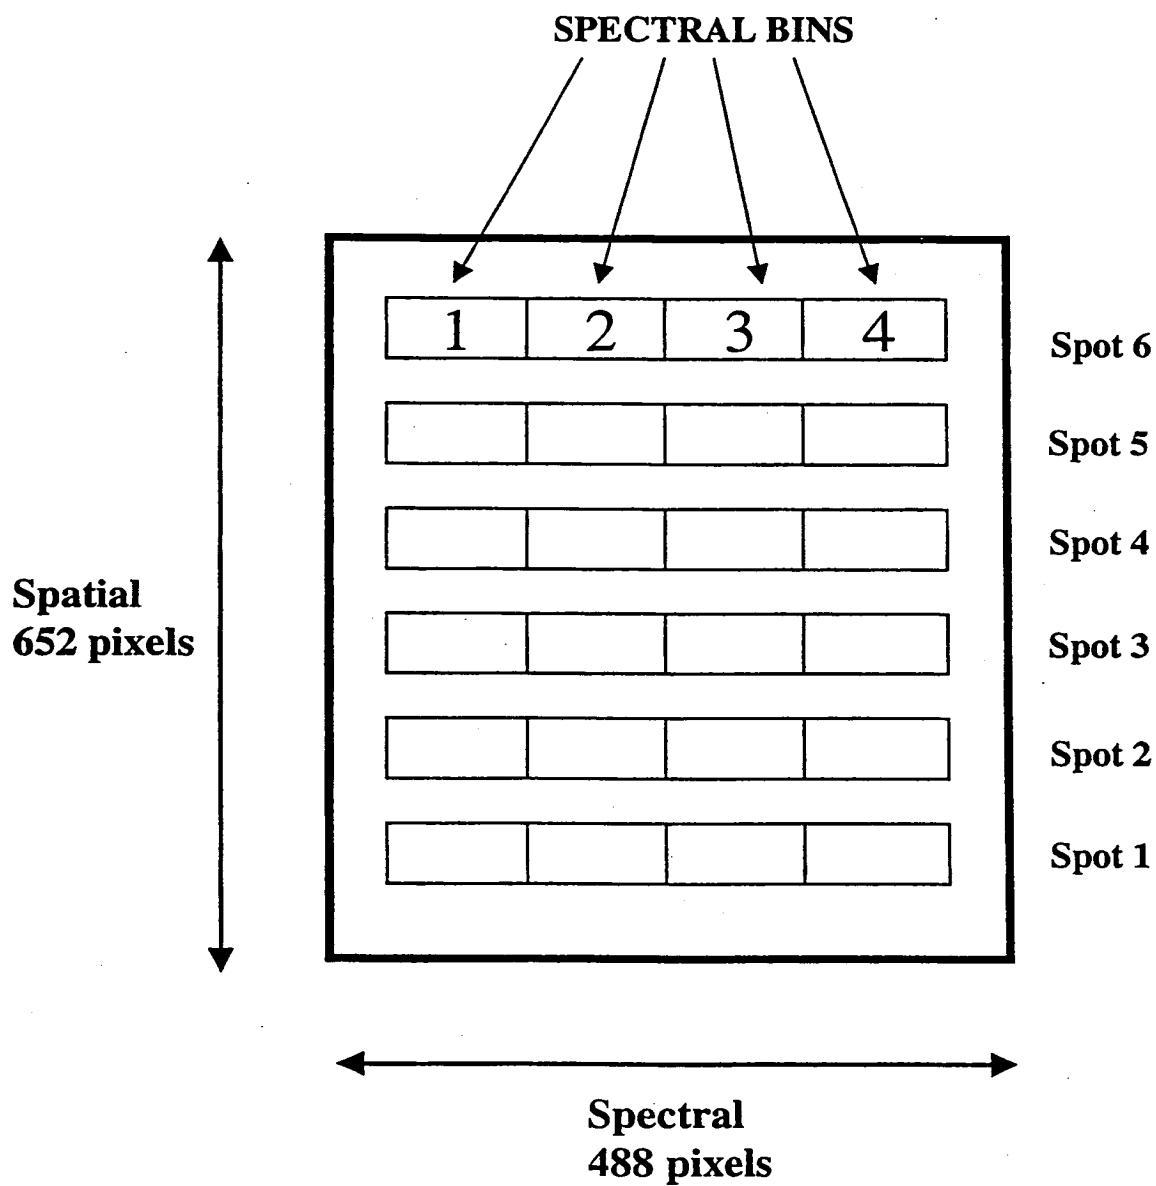


Fig. 6

7/9

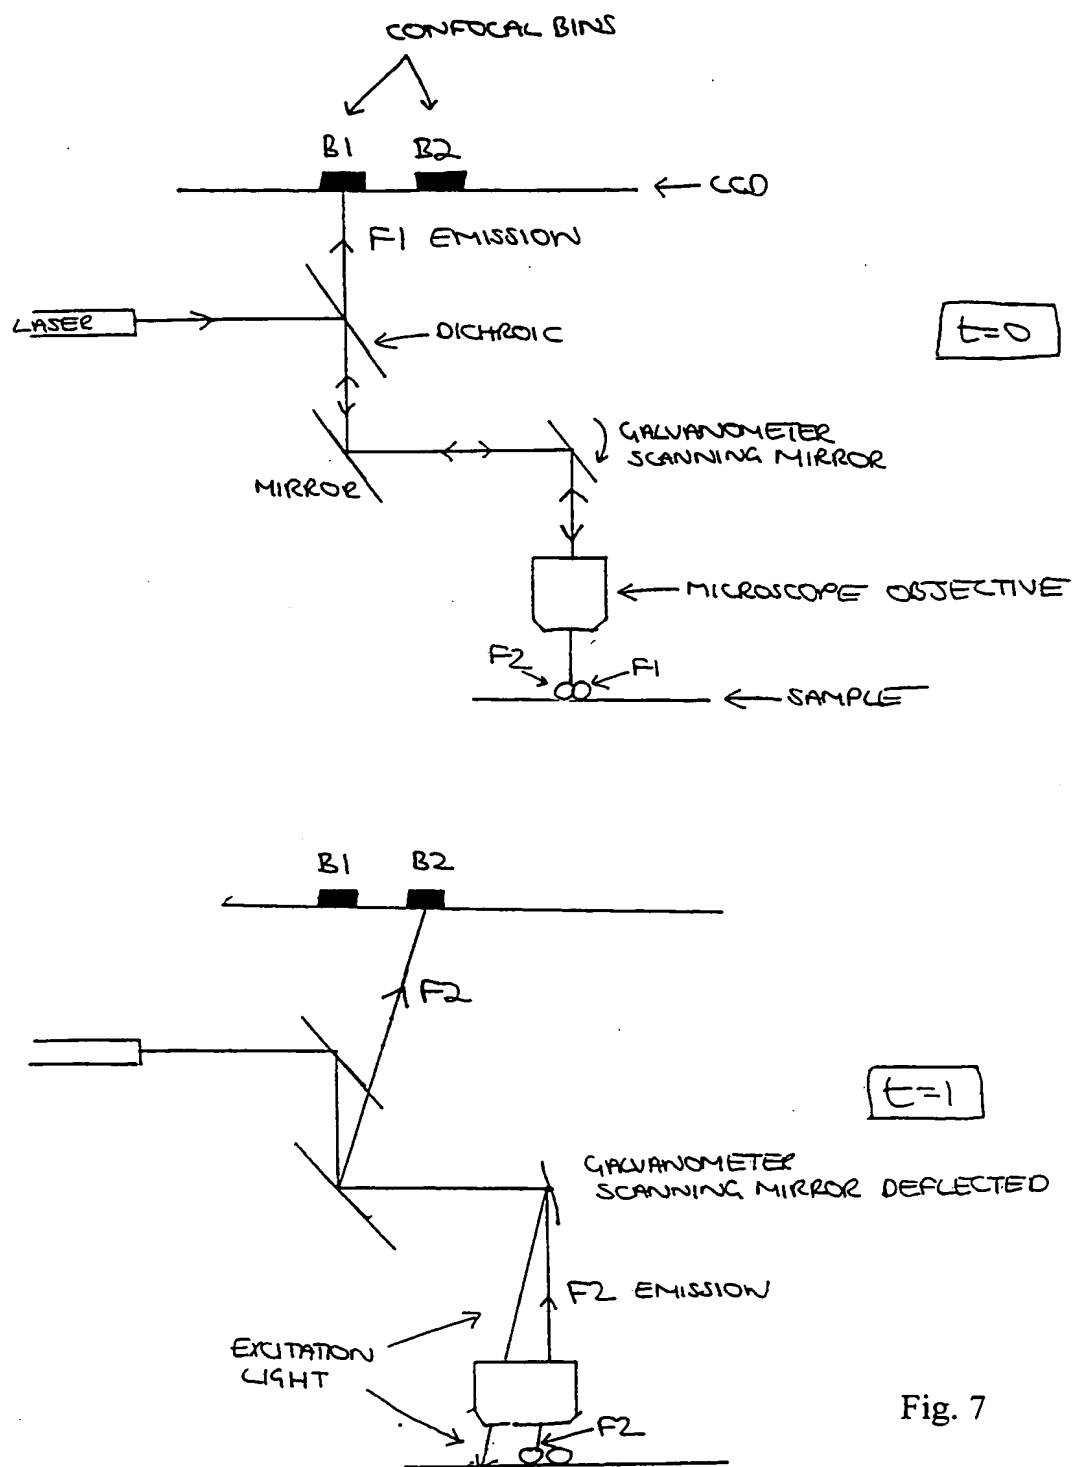


Fig. 7

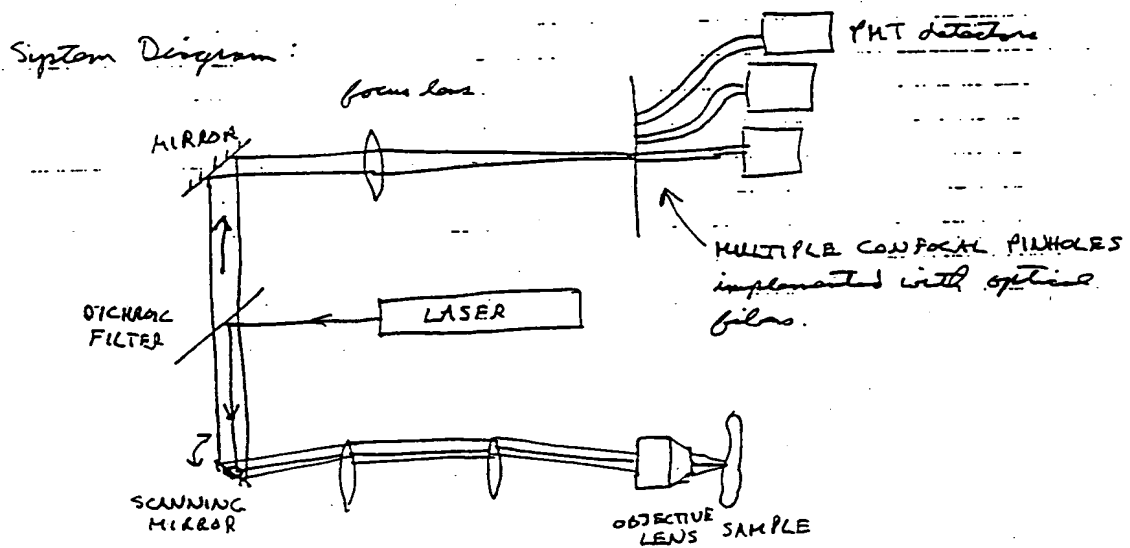


Fig. 8

NON EPI-ILLUMINATION SPOT ARRAY SYSTEM IAN WALTON 8/10/99

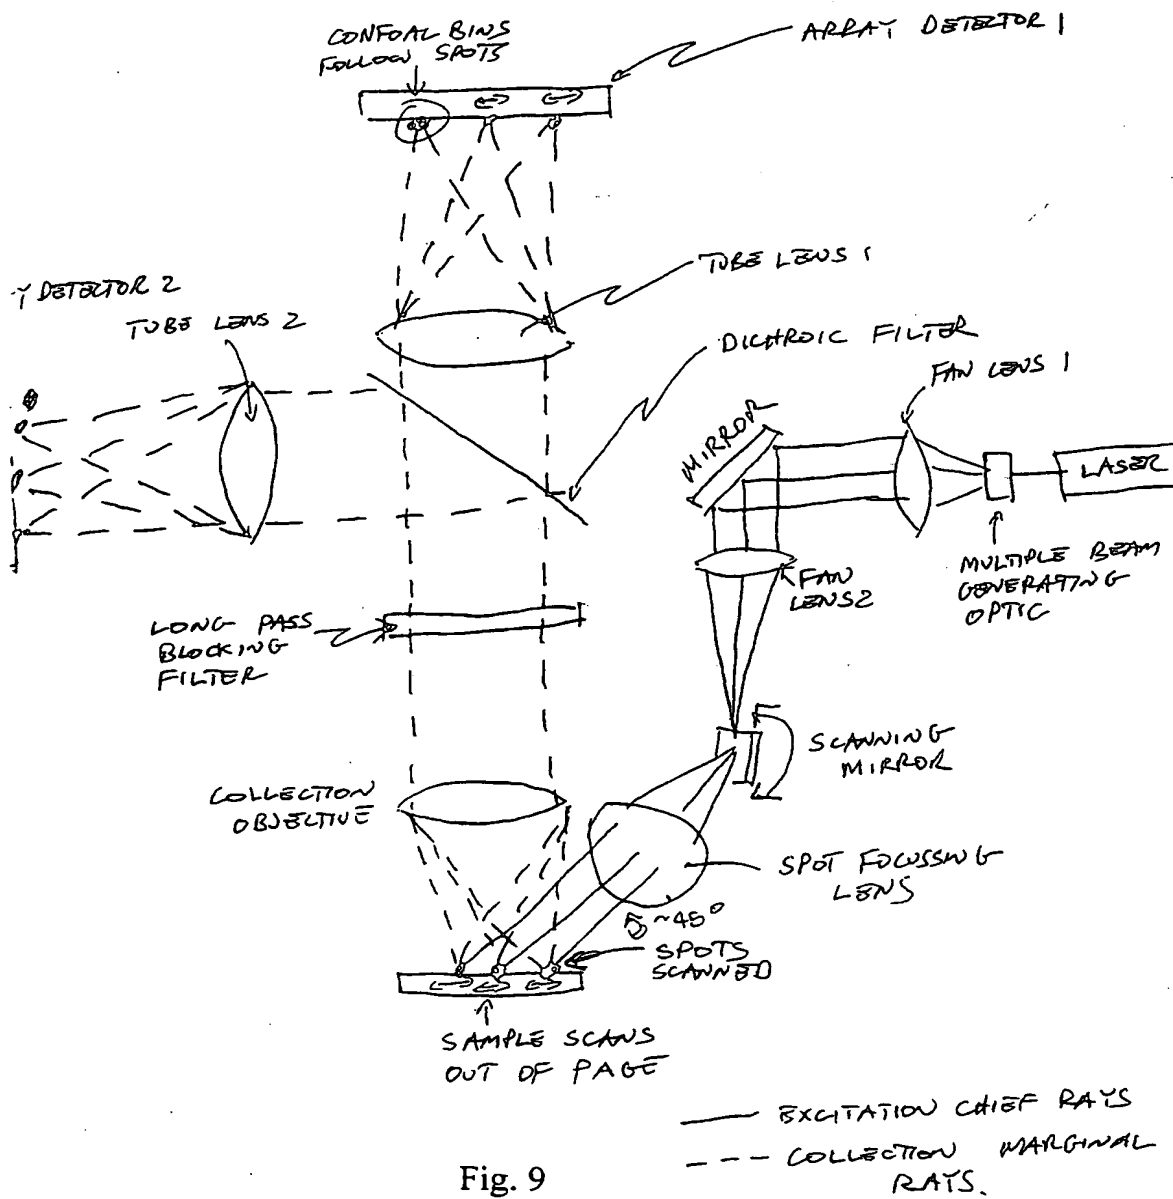


Fig. 9




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification: G01N 21/64		(11) International Publication Number: WO 00/11024
A3		(43) International Publication Date: 2 March 2000 (02.03.00)
(21) International Application Number: PCT/US99/19374 (22) International Filing Date: 20 August 1999 (20.08.99) (30) Priority Data: 60/097,506 21 August 1998 (21.08.98) US (71) Applicant: SURROMED [US/US]; 1060 East Meadow Circle, Palo Alto, CA 94303 (US). (72) Inventors: DIETZ, Louis, J.; 550 S. Shoreline Boulevard, Mountain View, CA 94041 (US). WALTON, Ian; 346 Lakeview Way, Redwood City, CA 94062 (US). NORTON, Scott; 600 Rainbow Drive, #149, Mountain View, CA 94041 (US). (74) Agents: SWANSON, Barry, J. et al.; Swanson & Bratschun, L.L.C., Suite 200, 8400 E. Prentice Avenue, Englewood, CO 80111 (US).		(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i> (88) Date of publication of the international search report: 29 June 2000 (29.06.00)

(54) Title: NOVEL OPTICAL ARCHITECTURES FOR MICROVOLUME LASER-SCANNING CYTOMETERS

(57) Abstract

Instrumentation and methods for performing charged coupled device (CCD) based confocal spectroscopy with a laser spot array are provided. A sample is scanned by a plurality of excitation laser scanning spots. The scanning spots are generated, for example, by converting a laser excitation beam into an array of beams using a multiple beam generating optic, such as a Damann grating. Each scanning spot scans and excites a separate region of the sample. Fluorescent light emitted by the sample is collected and imaged onto the surface of a CCD detector that has been electronically divided into bins of pixels, with each bin corresponding to one of the scanning spots. Each bin functions as a confocal aperture in which the confocal depth of focus can be controlled by changing the dimensions of the bin. Plural CCD detectors can be used for multichannel imaging of individual wavelengths. The instrumentation and methods are useful in any spectroscopic application including microscopy and microvolume laser scanning cytometry (MLSC).

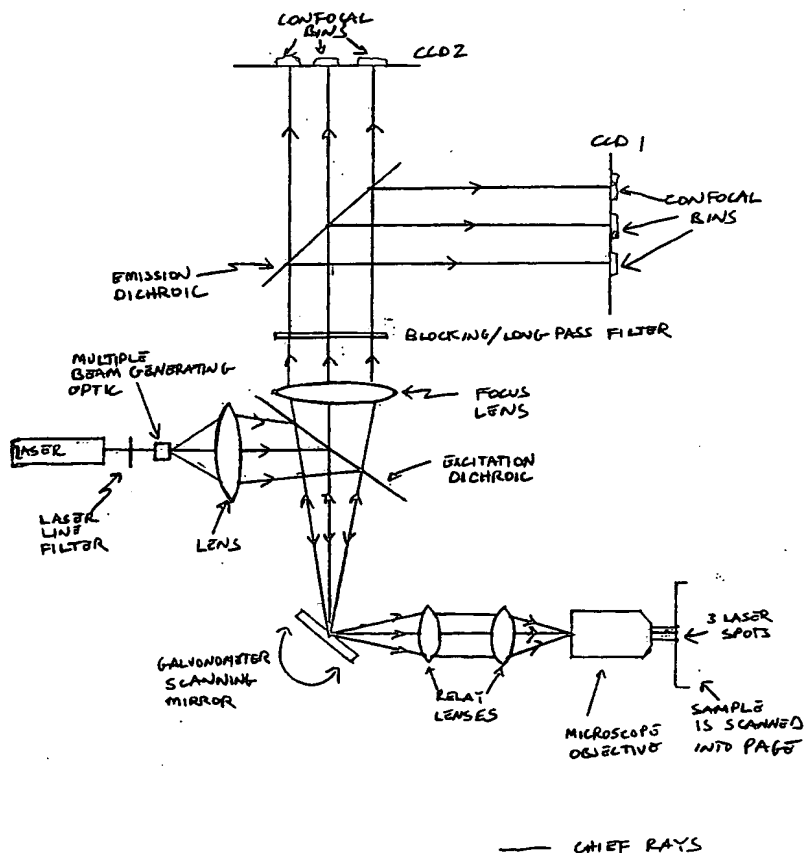

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US99/19374

A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) :G01N 21/64

US CL :250/226, 234, 208.2; 356/246, 317, 319, 326, 440

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : Please See Extra Sheet.

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5,726,751 A (ALTENDORF ET AL) 10 MARCH 1998 (10/03/98), SEE ENTIRE DOCUMENT.	1-30
A	US 5,446,532 A (YAMAZAKI) 29 AUGUST 1995 (29/08/95), SEE ENTIRE DOCUMENT.	1-30



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

23 FEBRUARY 2000

Date of mailing of the international search report

28 MAR 2000

Name and mailing address of the ISA/US
Commissioner of Patents and Trademarks
Box PCT
Washington, D.C. 20231
Facsimile No. (703) 305-3230

Authorized officer

JOHN LEE

Telephone No. (703) 308-0936

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US99/19374

B. FIELDS SEARCHED

Minimum documentation searched

Classification System: U.S.

250/226, 234, 208.2; 356/246, 317, 319, 326, 338, 440; 250/208.1, 235, 236, 484.4; 356/244, 73, 311, 318, 320, 331, 335, 336, 337, 339, 340, 341, 342, 343